

# SERVICE INFORMATION LETTER

AVOX Systems Inc., 225 Erie Street, Lancaster NY 14086-9502 USA  
Tel: 716-683-5100 • Fax: 716-681-1089 • Vendor Code: 53655

## **EQUIPMENT/FURNISHINGS - ATA CHAPTER 25**

### **MANUFACTURER VOLUNTARILY RECALLS POTENTIALLY CONTAMINATED POVIDONE IODINE PREP PADS THAT MAY BE CONTAINED IN AVOX SYSTEMS FIRST AID KITS**

**WARNING: USE OF CONTAMINATED POVIDONE IODINE PREP PADS MARKED AS AVOX SYSTEMS ANTISEPTIC APPLICATOR PADS PART NUMBER (PNR) 70135-00 AND POTENTIALLY CONTAINED IN AVOX SYSTEMS FIRST AID KITS COULD LEAD TO LIFE THREATENING INFECTION ESPECIALLY IN POPULATIONS AT RISK, INCLUDING NEONATES, IMMUNE-SUPPRESSED AND SURGICAL PATIENTS.**

#### 1. BACKGROUND

H&P Industries, Inc. has issued a voluntary recall of Povidone Iodine Prep Pads. These pads are potentially contaminated by ElizabethKingia meningosepticum which is a bacterium that can cause serious infection and death.

Some of these pads were packaged by H&P Industries for North Safety Products, then re-identified by AVOX Systems as Antiseptic Applicators PNR 70135-00 (see Table 1 and Figure 1). These antiseptic applicators are contained in the AVOX Systems first aid kits identified in Table 2.

#### 2. DESCRIPTION

A typical pair of PVP Iodine Wipes is shown in Figure 2.

These wipes are packaged 10 to a box by North Safety Products, re-identified by AVOX Systems and included in AVOX Systems first aid kits. The quantities of boxes (AVOX PNR 70135-00) in each AVOX first aid kit are listed by PNR in Table 2.

It is necessary to inspect all AVOX Systems first aid kits listed in Table 2 to determine if any contain the affected lots of PVP iodine wipes identified in Table 3. These affected lots show expiration dates between March 2011 and April 2014 (see Table 4). Figure 3 shows where the lot number appears. Figure 4 shows where the expiration date appears.

All affected units must be returned to AVOX Systems for proper disposal. Replacement units will be provided by AVOX Systems free of charge.

You are authorized to make copies of this SIL and give them to other persons. If you copy this SIL, you must copy all of the SIL.

#### 3. EFFECTIVITY

##### A. Aircraft


AVOX Systems first aid kits can be installed in any commercial, corporate or general aviation aircraft.

##### B. Spares

This SIL also applies to all units held in spares.

Table 1  
Relationship of Products by Company

Company	Nomenclature	PNR
H&P Industries, Inc.	Povidone Iodine Prep Pads	N/A
	PVP Iodine Wipe	N/A
AVOX Systems	Antiseptic Applicator	70135-00

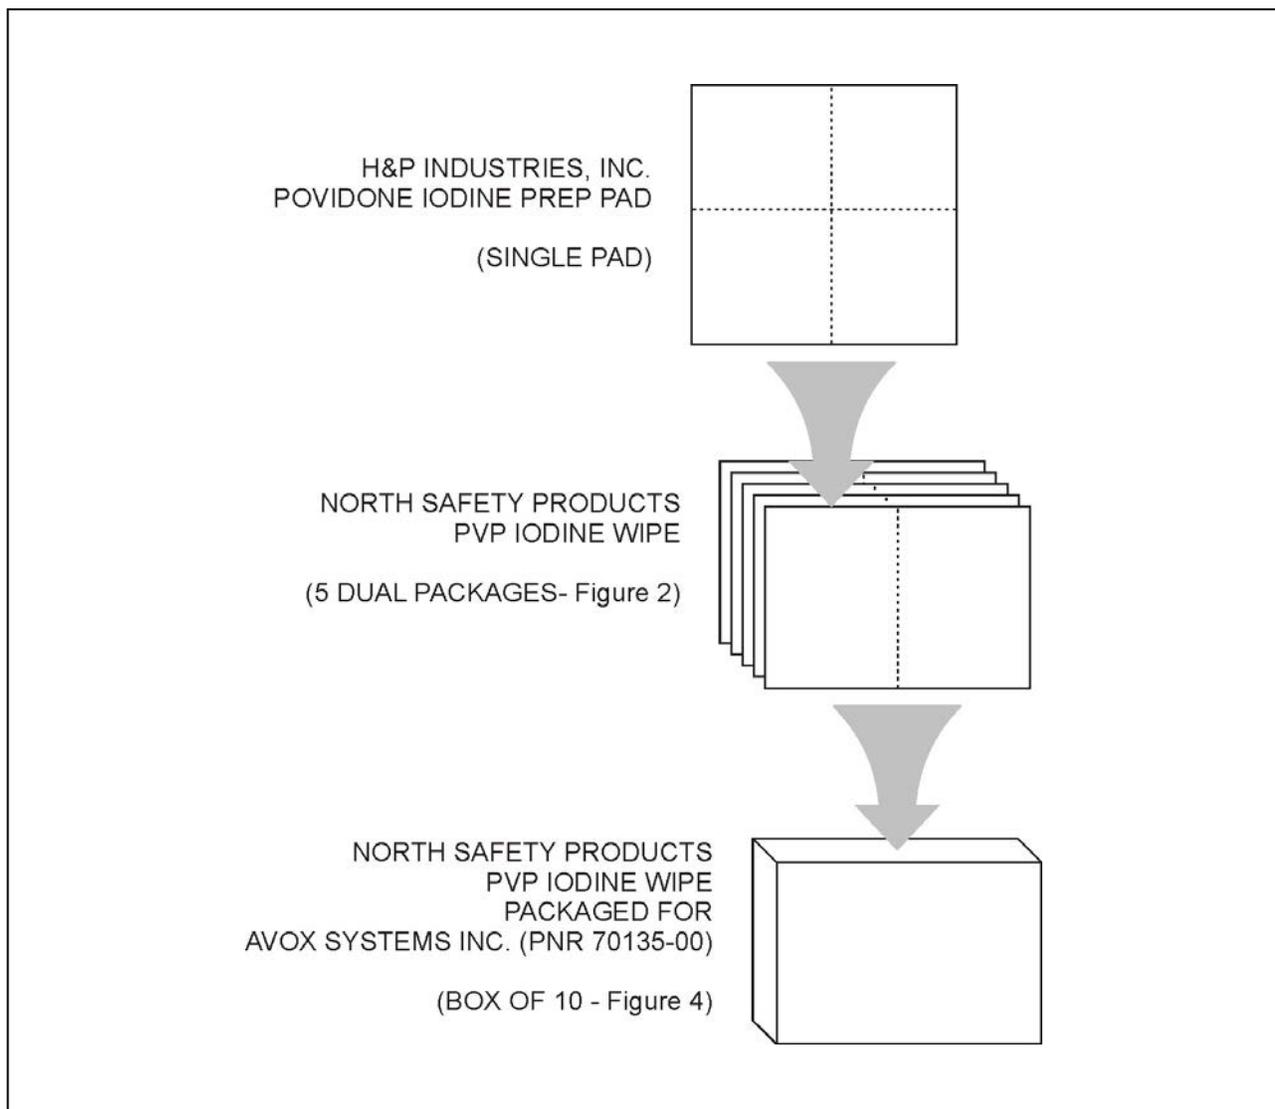

How the Product is Packaged  
Figure 1




Typical Pair of PVP Iodine Wipes Contained in AVOX Systems PNR 70135-00  
Figure 2

Table 2  
Part Numbers of Affected First Aid Kits

AVOX Part Number	Qty of Pads PNR 70135-00 per Kit
70001-00	2 boxes containing (10 each)
70002-00	4 boxes containing (10 each)
70003-00	6 boxes containing (10 each)
70004-00	2 boxes containing (10 each)
74050-00	2 boxes containing (10 each)
74051-00	4 boxes containing (10 each)
74052-00	6 boxes containing (10 each)
74052-01	2 boxes containing (10 each)
73777-01	2 boxes containing (10 each)

Table 3  
Affected Lot Numbers  
(See Figure 3)


8XXX
9XXX
0XXX
1XXX

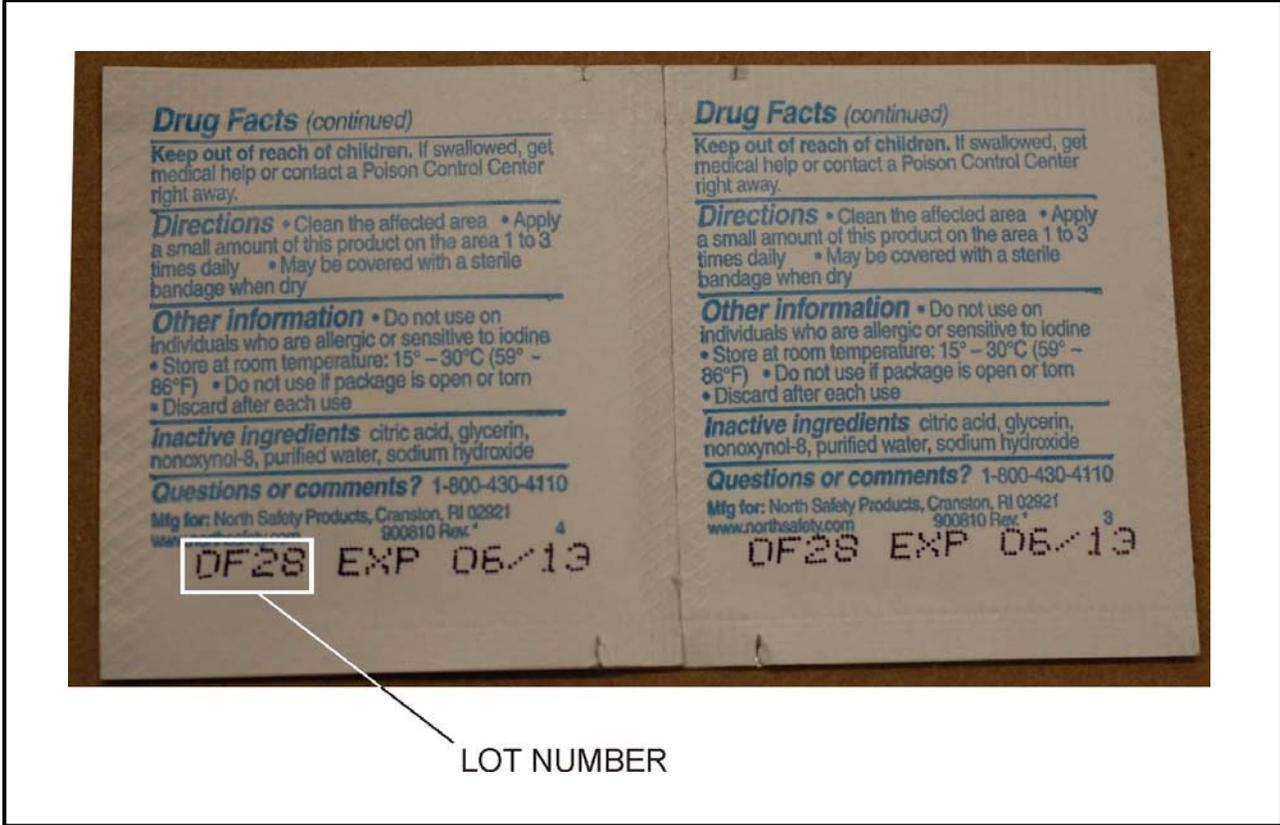

Example of Affected Lot Number  
Figure 3

Table 4  
Range of affected Expiration Dates  
(See Figure 4 for example)

Start Date	End Date
03/11	4/14

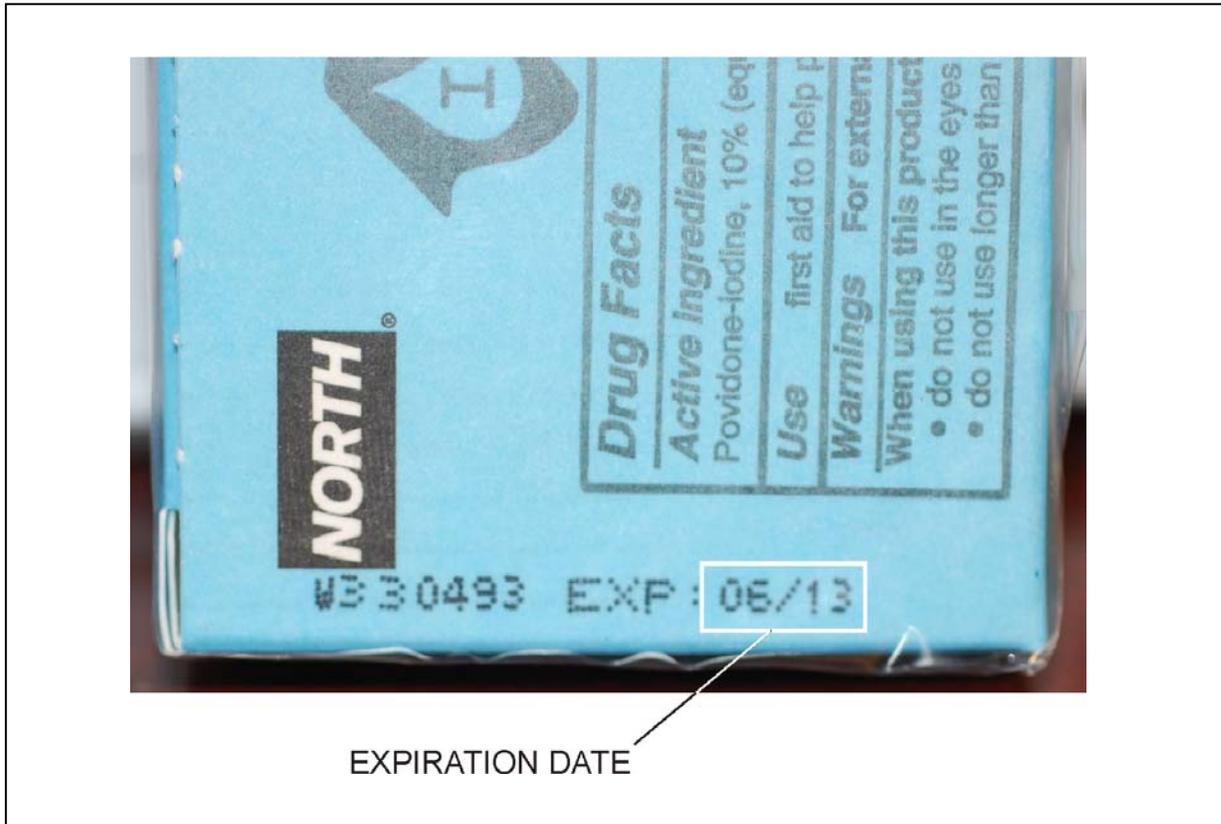

Example of Expiration Date on AVOX PNR 70135-00  
Figure 4

4. Action

- A. Immediately examine all AVOX Systems first aid kits (Table 2) on your fleet or in your stores.
- B. Quarantine all items affected by this SIL.
- C. Complete the form in the appendix of this SIL and email it to AVOX Systems to obtain replacement antiseptic applicators PNR 70135-00.
- D. Replace all units removed from first aid kits on aircraft and in stores with new antiseptic applicators obtained from AVOX Systems.
- E. The PVP Iodine Wipes have been designated as non- hazardous and can be disposed of through conventional methods.

5. APPENDIX

A. To get technical aid, contact a Zodiac Services location:

<b>ZODIAC SERVICES EUROPE</b>	<b>ZODIAC SERVICES ASIA</b>	<b>ZODIAC SERVICES AMERICAS</b>
Celine Melloul Product Support Manager 7, avenue du Parana BP 303 91958 COURTABOEUF cedex FRANCE Phone: +33 1 64 86 53 33 Fax: +33 1 64 86 69 85 celine.melloul@zodiac aerospace.com www.zodiac aerospace.com	Cyril Coutou Product Support Engineer 36 Loyang Drive SINGAPORE 508949  Phone : +65 6579 2251 Cell: +65 9770 5059 Fax: +65 6579 2231 cyril.coutou@zodiac aerospace.com www.zodiac aerospace.com	Ruben Membrila Technical Support Engineer 6734 Valjean Ave. Van Nuys, CA 91406 USA  Phone: +1 818 435 0928 x2928 Fax: +1 818 435 0960 ruben.membrila@zodiac aerospace.com www.zodiac aerospace.com

B. To buy spares or to have a cylinder assembly serviced, contact an Authorized Distributor:

<b>EUROPE: ZSE</b>	<b>UNITED KINGDOM: ZAU</b>	<b>USA: ZSU</b>
<b>ZODIAC SERVICES EUROPE</b> 7, avenue du Parana BP 303 91958 COURTABOEUF Cedex FRANCE Phone: +33 1 64 86 69 69 AOG: +33 1 49 75 45 73 Fax: +33 1 64 86 69 79	<b>ZODIAC Aerospace UK</b> Unit 9, Blackwell Drive Springwood Industrial Estate BRAINTREE Essex CM72QJ England Phone: +44 (0)1376 329 194 Fax: +44 (0)1376 340 734	<b>ZODIAC SERVICES AMERICAS</b> 4900 St Joe Boulevard Building 200, Suite 400 COLLEGE PARK, GA 30337 USA Phone: +1 678 228 8153 AOG: +1 800 879 0411 Fax: +1 818 994 7901
<b>MIDDLE EAST: ZSM</b>	<b>ASIA: ZSA</b>	
<b>IN-SERVICES MIDDLE EAST</b> Abu Dhabi International Airport Cargo Village Area P.O. Box 106675 ABU DHABI UNITED ARAB EMIRATES Phone: +(971)-2575 7088 AOG: +(971)-5064 20034 Fax: +(971)-2575 8482	<b>ZODIAC SERVICES ASIA</b> 36, Loyang Drive SINGAPORE 508949 Phone: +65 6546 9792 AOG: +65 9770 5061 Fax: +65 6579 2231	

## Notice of Destruction

### PRODUCT DESIGNATED FOR DESTRUCTION

**Product Description:** PVP -Iodine Prep Pads (AVOX P/N 70135-00 Applicator, Antiseptic)

<b>Item Number:</b>	AVOX P/N 70135-00	<b>If Applicable, NCR No.:</b>	
<b>Lot Code:</b>			
<b>Quantity/unit:</b>			

**Reason for Destruction:**

**Product Location:**

**Replacements shall be shipped to :**

**Name:**

**Address:**

**City:**

**State:**

**Zip Code:**

**Phone:**

**Email:**

**Contact Name:**

**NOTE:**  
**FIRST AID KITS (see notification letter) IDENTIFIED WITH LOT NUMBERS:**  
**W3500000, RW3500000, VW3500000**  
**OR HIGHER CONTAIN PVP -Iodine Prep Pads (AVOX P/N 70135-00 Applicator, Antiseptic)**  
**THAT ARE "ACCEPTABLE" FOR USE.**

### CERTIFICATE OF DESTRUCTION

**THIS PRODUCT HAS BEEN DESTROYED IN A MANNER RENDERING IT INCAPABLE OF USE.**

**Method of Destruction:**

- Deface and dispose of in accordance with local regulations.
- Other \_\_\_\_\_

**Note: The PVP Iodine Wipes have been designated as Non- hazardous and can be disposed of through conventional methods.**

**Destroyed By:**

**Title:**

**Verified By:**

**Title:**

Please email your completed form to Carol Messina, AVOX Customer Service Representative:  
 E-mail: carol.messina@zodiac aerospace.com